

A used needle may cause a needlestick injury, even if it is only exposed momentarily before being shielded. This may cause anxiety for healthcare professionals and patients alike.

Experience **safe** sampling

Variant	Size	Needle Length	Tube Length	Holder	Luer
With Luer Adapter 	20G / 0.9mm 21G / 0.8mm 22G / 0.7mm 23G / 0.6mm 25G / 0.5mm	19mm / 3/4"	200mm / 8" 300mm / 12"	—	✓
Without Luer Adapter 	20G / 0.9mm 21G / 0.8mm 22G / 0.7mm 23G / 0.6mm 25G / 0.5mm	19mm / 3/4"	200mm / 8" 300mm / 12"	—	—
With Pre-Attached Holder 	20G / 0.9mm 21G / 0.8mm 22G / 0.7mm 23G / 0.6mm 25G / 0.5mm	19mm / 3/4"	200mm / 8" 300mm / 12"	✓	✓

Accessory	Size	Needle Length	Accessory	Size
Luer Adapter 	21G / 0.8mm	19mm / 3/4"	Holder 	One Size

Sample with confidence

By utilising a user-centric design that provides protection once the needle is removed from the vein, **Unistik® ShieldLock** allows HCPs to draw large volumes of blood with ease.

Unistik® ShieldLock

Venous Safety Blood Collection

Sample with
confidence



Unistik®

Venous Safety Blood Collection

For more information, visit
owenmumford.com

© Copyright Owen Mumford 2022
SHIELDLOCK-GLT/MCC/0422/01



IN-VEIN
ACTIVATION



SLIDE TO
SHIELD



FLIP TO
SHIELD

OWEN MUMFORD

Owen Mumford Ltd., Brook Hill, Woodstock, Oxfordshire OX20 1TU, United Kingdom
T: +44 (0)1993 812021 E: info@owenmumford.com owenmumford.com

OWEN MUMFORD



Multi-sampling Luer

- Allows multiple blood samples to be collected from one patient



Transparent tube holder

- Easy to see the collection tubes filling up with blood



Thumb-activated safety shield

- Safety mechanism activated once needle is removed from the vein to help prevent needlestick injuries
- Allows for large volumes of blood collection with ease and minimal discomfort
- Audible click signals the safety guard is activated and the needle is completely retracted and locked

DEHP free tubing

- Preserves the blood chemical and physiological composition



Needle

- Thin wall needle for faster blood collection



Wings

- Flexible, textured wings to ensure a secure grip throughout the procedure


Designed to provide protection once the needle is removed from the patient's vein using a thumb-activated safety mechanism.




Available in five needle gauges, one needle length and two tube lengths.



Blood Collection Set with Luer Adapter




Blood Collection Set without Luer Adapter




Blood Collection Set with Pre-Attached Holder


How to use

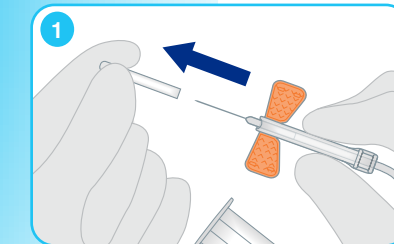

Remove needle sheath.

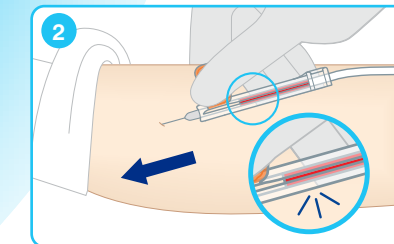


Hold wings and perform venipuncture, observe for blood flashback. Collect blood sample according to your facility's policy.

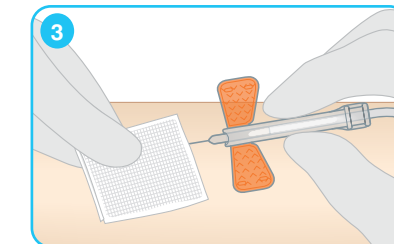

After completion of blood collection, gently remove needle from vein.



Slide translucent safety shield forward. With other hand, pull tubing backwards until an audible click is heard, indicating needle is completely retracted and locked.

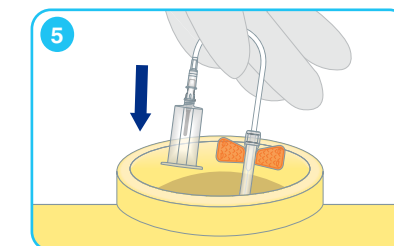

Dispose of all used materials as per your facility's policy.